590 FRANKLIN AVENUE
MOUNT VERNON, NY 10550
www.proactivemedical.com
855-237-7622

Sit-To-Stand Buttock Strap & Knee Strap Brace Instruction manual

SIT-TO-STAND SLING:

BUTTOCK STRAP INSTRUCTION

PLEASE SAVE THESE INSTRUCTIONS FOR FUTURE USE

⚠ **WARNING: Important! Read and understand these instructions before assembling or using the sling. If you do not understand any part of these warnings, cautions or instructions, contact a healthcare professional for direction in the use of this product. If the sling is not properly applied, personal injury and damage to the sling could result.**

⚠ **WARNING: If components are damaged or missing, contact your Proactive Medical authorized distributor immediately.**

⚠ **WARNING: Carefully inspect the sling before each use for wear and damage to seams, fabric, straps, and strap loops. Torn, cut, frayed or broken slings can fail, resulting in serious personal injury to the user. Use only slings that are in good condition. Discard and destroy old, unusable slings.**

⚠ **WARNING: DO NOT exceed the sling's maximum weight capacity.**

⚠ **WARNING: Notice for California Customers- California Proposition 65 WARNING: This product contains a chemical known to the State of California to cause cancer and reproductive or developmental harm.**

⚠ **WARNING: Proactive Medical Products assumes no responsibility for any damage or injury caused by improper application or use of this product.**

POSITIONING THE SLING

1. Check the patient's weight and the sling's maximum weight capacity. Ensure that the patient's weight does not exceed the sling's maximum weight capacity.

2. Review the following procedures carefully before attempting lift; call Proactive Medical's Technical Support at 845-205-6004 with any questions.

3. Use long loops, center loops, or short loops as shown in ***FIGURE 2***, to position Buttock Strap to provide the greatest support to the patient's middle and lower body during the following steps.

4. Attach Buttock Strap **strap A** to Sit-to-Stand Lift mast lower **loop a** as shown in ***FIGURES 1 and 3***.

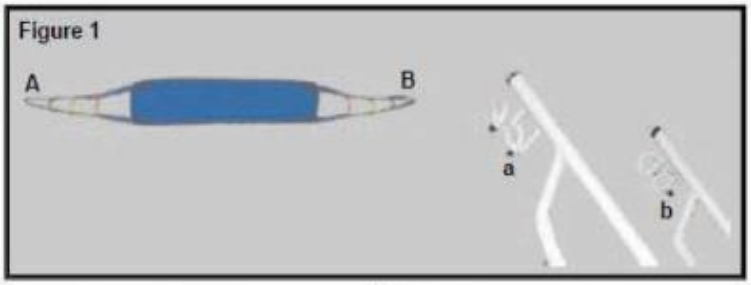

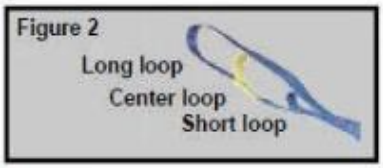

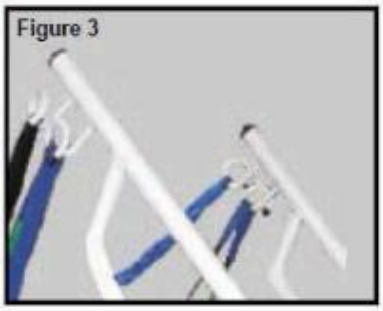

5. Bring Buttock Strap around the back of the patient's buttocks and attach Buttock Strap **strap B** to Sit-to-Stand Lift mast lower **loop b** as shown in ***FIGURES 1 and 3***.

6. Do not lock caster brakes in order to allow the lift to properly balance weight.

7. Proceed with lift and transfer as shown in ***FIGURE 4***.

SIT-TO-STAND SLING:

KNEE STRAP BRACE INSTRUCTION

PLEASE SAVE THESE INSTRUCTIONS FOR FUTURE USE

⚠ **WARNING: Important! Read and understand these instructions before assembling or using the Knee Strap Brace. If you do not understand any part of these warnings, cautions or instructions, contact a healthcare professional for direction in the use of this product. If the Knee Strap Brace is not properly applied, personal injury and damage to the brace could result.**

⚠ **WARNING: If components are damaged or missing, contact your Proactive Medical authorized distributor immediately.**

⚠ **WARNING: Carefully inspect the Knee Strap Brace before each use for wear and damage to seams, fabric, straps, and buckle. Do not use a damaged brace.**

⚠ **WARNING: Notice for California Customers - California Proposition 65 WARNING: This product contains a chemical known to the State of California to cause cancer and reproductive or developmental harm.**

⚠ **WARNING: Proactive Medical Products assumes no responsibility for any damage or injury caused by improper application or use of this product.**

Installing the Knee Strap Brace

1. Secure each side of the brace to the attachment point on the outer side of each knee pad using the hook-and-loop fasteners.

2. Place the patient's feet on the platform and their knees against the knee pads.

3. Center the blue padded section behind both lower legs, just below the knees.

4. Fasten both buckles and adjust the straps evenly until the brace is snug but comfortable.

5. Confirm that the padding is centered, the straps are not twisted, and both buckles are fully secured.

Proceed with the sit-to-stand transfer as directed by the healthcare provider.

Proactive medical products

SIT-TO-STAND SLING:

PLEASE SAVE THESE INSTRUCTIONS FOR FUTURE USE

Washing Instructions:

1. Machine wash warm or cold
    a. Maximum washing temperature 185°F (85°C)
    b. Wash at 160°F (71°C) for 3 minutes
    c. Wash at 145°F (63°C) for 10 minutes
    d. Air dry, or tumble dry at cool or very low temperature
    e. Do not tumble dry at high temperature
2. Use non-enzyme detergent
3. Do not use bleach
4. Do not wash with other colors

⚠ **WARNING: After each laundering (in accordance with instructions on the sling), inspect sling(s) for wear, tears, and loose stitching. Bleached, torn, cut, frayed, or broken slings are unsafe and could result in injury. Discard immediately.**

LIMITED LIFETIME WARRANTY:

Your Proactive Medical sling product is warranted to be free of defects in materials and workmanship for the lifetime of the original consumer purchaser. Useful life of this product is six months from date of purchase under normal use, however, heavy use or excessive washing may reduce the useful life of the product. In the event of a defect covered by this warranty, we will, at our option, repair or replace the device. This warranty does not cover device failure due to owner misuse or negligence, or normal wear and tear.

Sling Material: Polyester / Straps Material: Polypropylene